

Predict

DDBSP – Dortmund Data Bank Software Package



DDBST - Dortmund Data Bank Software & Separation Technology GmbH

Marie-Curie-Straße 10

D-26129 Oldenburg

Tel.: +49 441 361819 0

support@ddbst.com

www.ddbst.com

Contents

1	Introduction	3
1.1	Supported Data Types	3
1.2	Supported Group Contribution Models	3
1.3	Supported Cubic EOS Mixing Rules	3
1.4	Supported Group Contribution Equation of State Models	4
2	Menu	5
2.1	Component List	6
2.2	Data Type and Model Settings	7
3	Calculation	9
3.1	Vapor-Liquid Equilibria	9
3.1.1	2/3 Flash	9
3.1.2	VLE	11
3.1.3	Henry	13
3.1.4	Phase Envelope	14
3.2	Solubility	15
3.2.1	SCF	15
3.2.2	SLE	16
3.2.3	LLE	17
3.3	Activity	18
3.3.1	ACT	18
3.3.2	ACT_inf	19
3.3.3	ACT_inf_all	21
3.4	Excess properties	23
3.4.1	HE	23
3.4.2	VE	24
3.4.3	CPE	25

1 Introduction

Predict is a program to calculate different data types by a large variety of models.

1.1 Supported Data Types

Predict can calculate the following data types:

1. Vapor Liquid Equilibria
 - a. 2/3 Flash
 - b. VLE (Vapor-Liquid Equilibrium)
 - c. Henry
 - d. Phase Envelope
2. Solubility
 - a. SCF (Solubility in supercritical fluids)
 - b. SLE (Solid-Liquid Equilibrium)
 - c. LLE (Liquid-Liquid Equilibrium)
3. Activity
 - a. ACT (Activity coefficients at given concentrations)
 - b. ACT_inf (Activity coefficients at infinite dilution)
 - c. ACT_inf_all (Activity coefficient of given components with a list of solvents at infinite dilution)
4. Excess Properties
 - a. HE (Excess enthalpy)
 - b. VE (Excess volume)
 - c. CPE (Excess heat capacity)

1.2 Supported Group Contribution Models

Predict support the group contribution models UNIFAC, mod. UNIFAC(Do.), NIST mod. UNIFAC and mod. UNIFAC (Ly).

1.3 Supported Cubic EOS Mixing Rules

Predict supports the cubic equation of state models Soave-Redlich-Kwong (SRK), Peng-Robinson (PR), Peng-Robinson 1978 (PR78) and Redlich-Kwong (RK).

As K_{ij} mixing rules the quadratic mixing rule and Panagiotopoulos/Reid are supported. In this case the following temperature function is used:

$$K_{ij}[K] = a_{ij} + b_{ij}T + c_{ij}T^2 + \frac{d_{ij}}{T} + \frac{e_{ij}}{T^2}$$

As g^E mixing rules Vidal, Tochigi, Michelsen, PSRK, VTPR and LCVM are supported. In this case the following temperature function is used:

$$G_{ij} = \exp\left(-\frac{T_{ij}}{RT}\right)$$

$$T_{ij}[\text{cal/mol}] = a_{ij} + b_{ij}T + c_{ij}T^2 + \frac{d_{ij}}{T} + e_{ij}T \cdot \ln(T) + f_{ij}T^3$$

The supported g^E models for the mixing rule are NRTL, Wilson, UNIQUAC, NRTL (Vidal) and UNIQUAC (res.).

For Soave-Redlich-Kwong and Peng-Robinson the original alpha functions (using the acentric factor ω), Mathias-Copeman¹ and Twu-Bluck-Cunningham-Coon² are supported. The Stryjek-Vera³ alpha function is available for Peng-Robinson only.

1.4 Supported Group Contribution Equation of State Models


Predict supports the group contribution equation of states PSRK, PSRK2 and VTPR.

¹ Mathias P.M., Copeman T.W., "Extension of the Peng-Robinson Equation of State to Complex Mixtures: Evaluation of the Various Forms of the Local Composition Concept", Fluid Phase Equilib., 13, 91-108, 1983

² Twu C.H., Bluck D., Cunningham J.R., Coon J.E., "A Cubic Equation of State with a New Alpha Function and a New Mixing Rule", Fluid Phase Equilib., 69, 33-50, 1991

³ Stryjek R., Vera J.H., "PRSV: An Improved Peng-Robinson Equation of State for Pure Compounds and Mixtures", Can.J.Chem.Eng., 64, 323-333, 1986

2 Menu

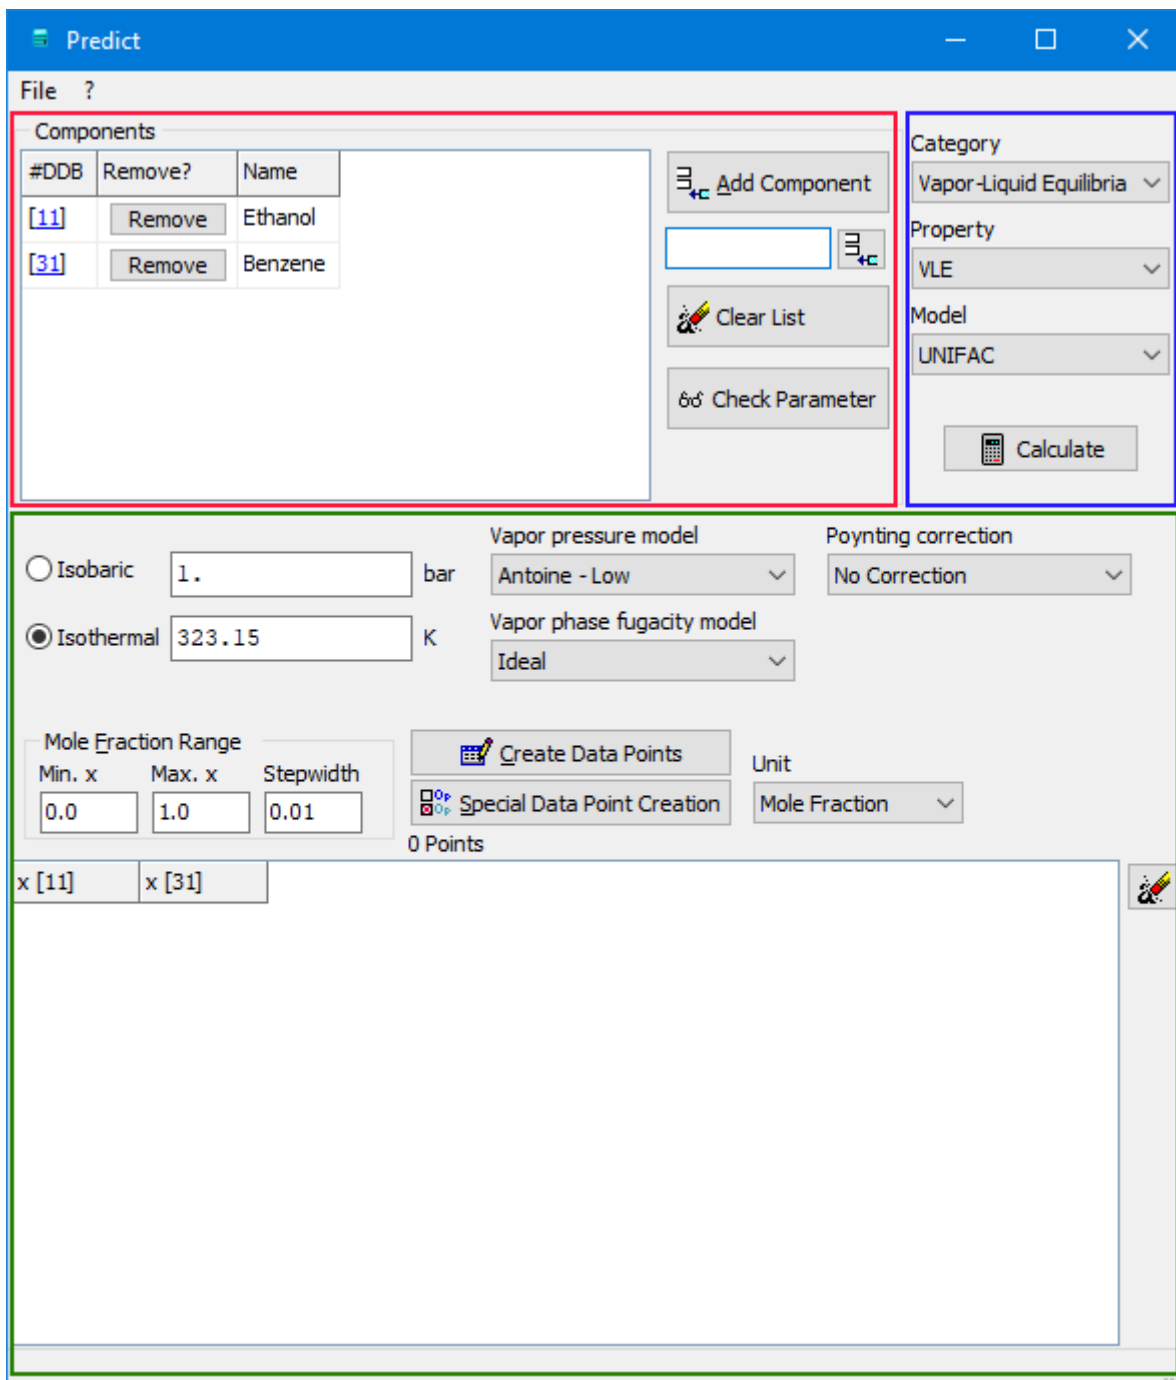

The menu has the following main parts:

1. List of components (red)
2. Data type and model settings (blue)
3. Specific data type calculation options (green)

2.1 Component List

The list of components displays the current system, which should be calculated. New Components can be added by using the “Add Component” button. This will open the component selection.

Component Selection

File Edit ?

Names: (Substrings combined by &(and), |(or), !(not), typing a number -> switch to DDB number/s selection)

Search <Names>

Reload Result List from History

Clear History

Search Item: Names

Search Type: Search in Active List Search Complete Database

Found Components: Clear List

Number	Type	Loc.	Name	Formula	CAS-RN	Mol. Weight
1	C	DDB	Acetaldehyde	C2H4O	75-07-0	44.053
2	C	DDB	Acetamide	C2H5NO	60-35-5	59.068
3	C	DDB	Acetonitrile	C2H3N	75-05-8	41.053
4	C	DDB	Acetone	C3H6O	67-64-1	58.080
5	C	DDB	Ethylenediamine	C2H8N2	107-15-3	60.099
6	C	DDB	1,2-Dibromoethane	C2H4Br2	106-93-4	187.862
7	C	DDB	Ethyl bromide	C2H5Br	74-96-4	108.966
8	C	DDB	1,2-Ethanediol	C2H6O2	107-21-1	62.068
9	C	DDB	Ethyl iodide	C2H5I	75-03-6	155.966
10	C	DDB	5-Ethyl-2-nonanol	C11H24O	103-08-2	172.311
11	C	DDB	Ethanol	C2H6O	64-17-5	46.069

Select Component [C1]

Add Component [C1] to DDB Query


Display Options: Normal Components Salts Adsorbents Polymers Complete Data Public DB Private DB Synonyms

Search Options: Synonyms

Cancel


Public Folder C:\DDBMAIN\DC Private Folder C:\DDBMAIN\DDBPI 79313 components

Components can also be added by typing the DDB numbers in the field beneath the “Add Component” button and confirming the numbers by using the button. “Clear List” removes all components from the list. The “Remove” button deletes one specific component. A list of components can be loaded by the “Open System” option in the “File” menu. It is also possible to save the current system with the “Save System” option. The “Check Parameters” button opens an extra menu for the parameter check. The “Overview” tab shows for which model all needed parameters are given for the defined component system. A more comprehensive view can be found in the “Details” tab.

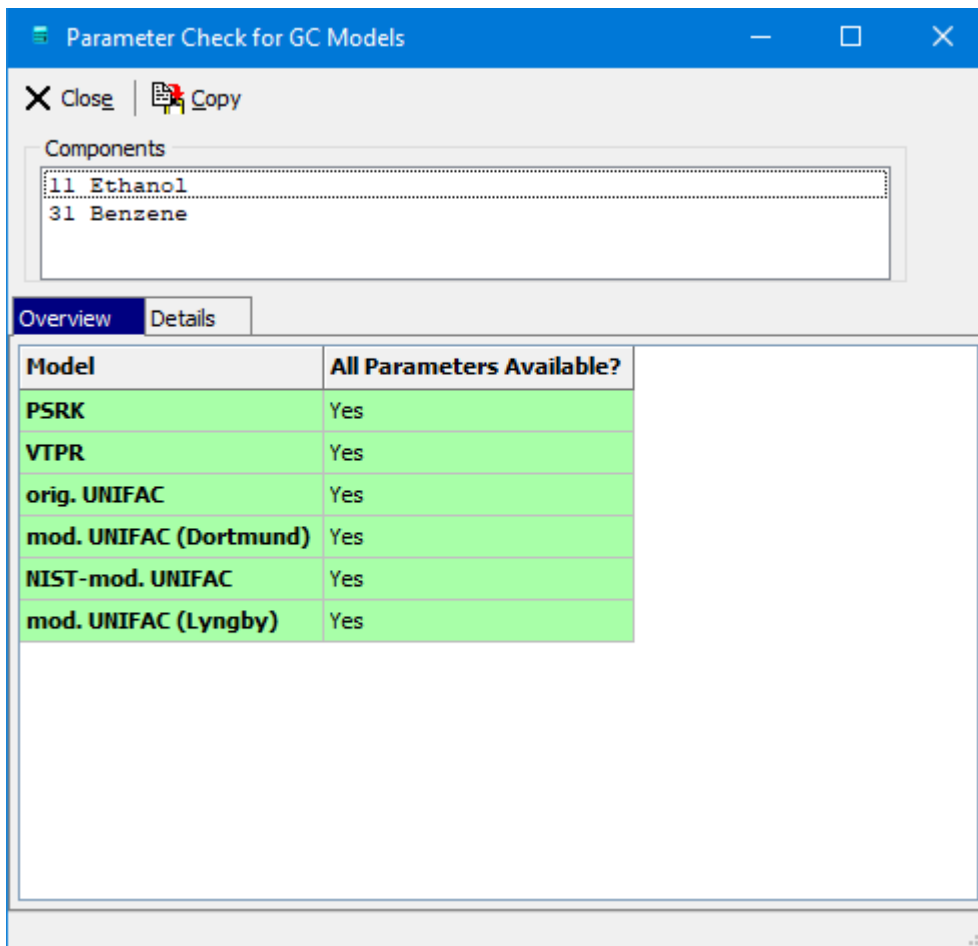


2.2 Data Type and Model Settings

The general options of the calculation are in the upper right corner of the menu. Predict is able to calculate a large amount of data types. So, data types are categorized for reasons of clarity. After a suitable category is chosen, the user can select the right property from the menu. Further calculation options are given at the bottom of the menu after the property selection. The last dropdown menu allows the selection of the model.



The “Calculate” button starts the calculation. In a case of an EOS model selection a further menu for EOS options and parameter selection will open.

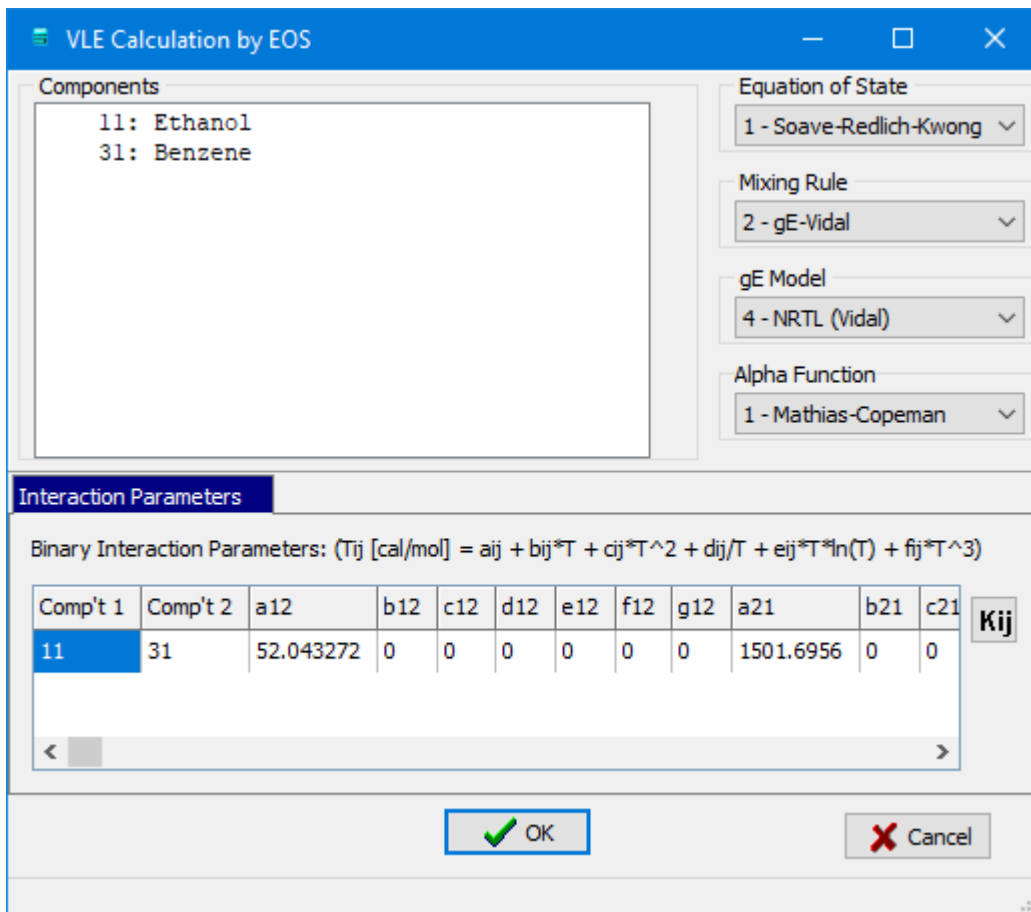

In this menu the Equation of State, the Mixing Rule, the gE Model and the Alpha Function can be selected. The Parameters can then be set by hand or by using the “Kij” button. This option allows to select parameters from the library or from a project file. If there are already recommended parameters in the library, they will automatically loaded to the menu.

3 Calculation

The Predict program gives further calculation options for every property at the bottom of the menu

3.1 Vapor-Liquid Equilibria

3.1.1 2/3 Flash

The 2/3 Flash program can calculate the phase split for a given feed concentration at the given temperature and pressure. This calculation needs an equation of state as basis model.

The options on the top left allows to define a constant temperature or pressure and an associated temperature or pressure range. A vapor-liquid or a vapor-liquid-liquid flash can be selected with the “Flash Type” Combo box on the right. The box beneath activates the PSRK Volume correction. In the “Feed Compositions” box the concentrations for the calculation are stored, either in mole fractions or weight fractions. Further columns are added by using the *Enter* key in the last row.

Result

The result table starts with small list of the used components. This is followed by a model dependent list of constants and parameters, which are used for the calculation.

T [K] = 323 P [bar] = 0.44											
No.	#DDB	z(i)-Feed	Given Feed N(i)-Feed	x(i)-Phase 1	N(i)-Phase 1	Liquid phase phi(i)-Phase 1	y(i)-Phase 2	N(i)-Phase 2	Vapor phase phi(i)-Phase 2	Fug(i) [bar]	
1	11	2.000000e-01	2.000000e-01	6.549702e-02	8.334671e-03	3.319941e+00	2.196115e-01	1.916653e-01	9.901406e-01	9.567635e-02	
2	31	8.000000e-01	8.000000e-01	9.345030e-01	1.189180e-01	8.226038e-01	7.803885e-01	6.810820e-01	9.850551e-01	3.382393e-01	
			1			0.127253			0.872747		
			71.7047			9.67309			62.0316		
						0.0994136			60.1793		
						0.00162887			0.986024		
						0.764632			0.00119107		
						-32797.7			-104.464		
						-100.677			-0.207624		

The result table shows detailed information about the used feed concentration and the resulting phases at the given temperature and pressure. The table shows the state of the given phases and gives information about concentration, amount of the component and the fugacity coefficients. Further information are given below the small tables. The following tables explains the abbreviations.

Abbreviations in the table:

Short Term	Description
i	Component (numbering order from top to bottom as in the main form's component list)
z(i)	Mole fraction of component I in the feed
x(i)	Mole fraction of component I in the liquid phase
y(i)	Mole fraction of component I in the vapor phase
F	Total feed (1 mole)
N(i)	Total number of moles of component I in the described phase (Total feed 1 mole)
phi(i),L	Liquid phase fugacity coefficient
phi(i),V	Vapor phase fugacity coefficient
Fug(i)	Fugacity $f = \Phi_{L,i} \cdot x_i \cdot P$ $f = \Phi_{V,i} \cdot y_i \cdot P$

Abbreviations below the table:

Short Term	Description
N	Amount of substance of the phase (complete, liquid phase, vapor phase)
M	Mass (complete, liquid phase, vapor phase)
V	Volume (liquid phase, vapor phase)
Z	Compressibility (liquid phase, vapor phase)
V (Penelouxcorr.)*	Volume (liquid phase, vapor phase)
Rho (Penelouxcorr.)*	Density (liquid phase, vapor phase)
h-h0	Real part of enthalpy (liquid phase, vapor phase, complete system)
s-s0	Real part of entropy (liquid phase, vapor phase, complete system)

*"Penelouxcorr." means that the Peneloux correction for the density was taken into account.

3.1.2 VLE

The screenshot shows the VLE calculation interface. It includes the following elements:

- Conditions:** Radio buttons for **Isobaric** (1. bar) and **Isothermal** (323.15 K).
- Vapor pressure model:** Dropdown menu set to **Antoine - Low**.
- Poynting correction:** Dropdown menu set to **No Correction**.
- Vapor phase fugacity model:** Dropdown menu set to **Ideal**.
- Mole Fraction Range:** Input fields for **Min. x** (0.0), **Max. x** (1.0), and **Stepwidth** (0.1).
- Buttons:** **Create Data Points** and **Special Data Point Creation**.
- Unit:** Dropdown menu set to **Mole Fraction**.
- Table:** A table with 66 points. The first row is highlighted in blue and yellow, showing values 0.0, 0.0, and 1.0 for columns x [11], x [31], and x [161] respectively. The second row shows 0.0, 0.1, and 0.9.

A constant pressure or a constant temperature can be specified for the VLE calculation. It is also possible to define the liquid concentrations for the calculation. These points can either be created by using the “Create Data Points” or “Special Data Point Creation” button. The first option uses the Mole Fraction range and creates with the limits and step width on the left side the desired concentrations. The second option uses an extra menu with more options for ternary and higher systems. This menu also allows to create concentrations by hand. If no concentrations are given in the feed, the program will create concentrations with the help of the first option. If a group contribution model is chosen, further options for the vapor pressure model, the vapor phase fugacity model and the Poynting correction appear.

Vapor phase fugacity model

Predict supports an ideal vapor phase but automatically switches to the Marek/Standart method for an internally stored list of carboxylic acids considering the vapor phase association.

The other methods include different cubic equations of state with the quadratic mixing rule and the Hayden-O-Connell method.

Vapor pressure model

The following pure component vapor pressure equations (see the PCPEquationFit documentation for the equation details) are supported:

1. Antoine – Low: This option searches the list of available Antoine parameter sets for that one which has the lowest lower validity range (this option was implemented to mimic the behavior of RecVal, which uses a low temperature and a high temperature set of Antoine parameters).
2. DIPPR 101 equation
3. Wagner equation (2.5-5 form)
4. Extended Antoine (Aspen)

Poynting Correction

The Poynting correction needs pure component densities resp. volumes v_i .

$$Poy_i = \exp \frac{v_i(P - P_i^S)}{RT}$$

Predict supports:

1. Densities calculated with the DIPPR 105 equation. These aren't original DIPPR parameters. The parameters are regressed by DDBST personnel with the help of the DDB pure component properties data bank (“PCP Equation Fit” program).

2. Densities by the Yen/Woods⁴ correlation.

Result

The result table starts with a small list of the used components. This is followed by a model dependent list of constants and parameters, which are used for the calculation. The results is given after that in table form.

I'x	T [K]	P [kPa]	x1 [mol/mol]	x2 [mol/mol]	y1 [mol/mol]	y2 [mol/mol]	Act.C.1[-]	Act.C.2[-]	phi.L.1[-]
1	323.150	36.362	0.00000	1.00000	0.00000	1.00000	7.52842	1.00000	6.08779
2	323.150	38.113	0.01000	0.99000	0.05452	0.94548	7.01718	1.00035	5.41398
3	323.150	39.616	0.02000	0.98000	0.09817	0.90183	6.56099	1.00137	4.87017
4	323.150	40.910	0.03000	0.97000	0.13380	0.86620	6.15221	1.00303	4.42238
5	323.150	42.029	0.04000	0.96000	0.16336	0.83664	5.78447	1.00527	4.04749
6	323.150	42.999	0.05000	0.95000	0.18823	0.81177	5.45243	1.00807	3.72922
7	323.150	43.842	0.06000	0.94000	0.20939	0.79061	5.15160	1.01140	3.45580
8	323.150	44.576	0.07000	0.93000	0.22758	0.77242	4.87816	1.01525	3.21851
9	323.150	45.218	0.08000	0.92000	0.24336	0.75664	4.62886	1.01957	3.01072
10	323.150	45.780	0.09000	0.91000	0.25717	0.74283	4.40091	1.02436	2.82736
11	323.150	46.273	0.10000	0.90000	0.26933	0.73067	4.19194	1.02961	2.66442

The table contains the following abbreviations.


Column	Description
I'x	Sequential number
T	Temperature
P	Pressure
x1	Liquid mole fraction of component 1 (carbon dioxide in this example)
y1	Vapor mole fraction of component 1
Act. C.1	Activity coefficient of component 1
phi. L.1	Liquid fugacity coefficient for component 1
phi. V. 1	Vapor fugacity coefficient for component 1
Fug 1	Fugacity for component 1
vv	Vapor volume
vl	Liquid volume
vE	Excess volume
hE	Excess enthalpy

The output is finished if a critical point has been identified or the complete composition range has been calculated. If an azeotropic point has been identified it will be displayed in the table. Beside these tables several plots are generated. These plots can be printed, saved and copied to the Windows clipboard.

⁴ Yen L. C., Woods S. S., "A Generalized Equation for Computer Calculation of Liquid Densities", AIChE J., 12(1), 95-99, 196

3.1.3 Henry

The Henry calculation only works for binary systems.

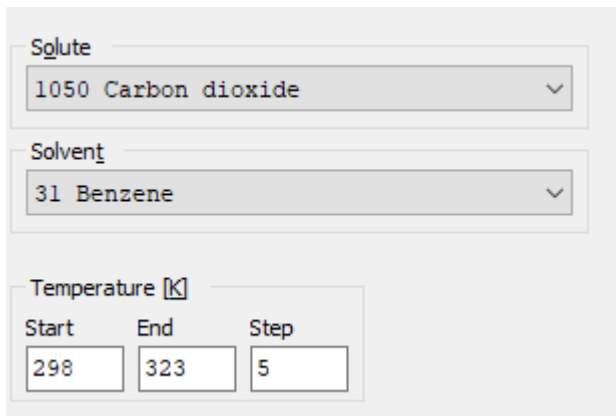

For the GLE (Gas-Liquid Equilibrium) calculation it has to be defined, which component is the liquid solvent. It is also necessary to define a vaporous component, which will solute in the solvent phase. At the bottom of the menu, the user defines a temperature range for the calculation.

Result

The results are shown after the component and parameter list.

Calculation of Henry coefficients
 Solute: 1050 Carbon dioxide
 Solvent: 31 Benzene

T [K]	H12 [bar]	Psat2 [bar]	vL [1/mol]	vV [1/mol]
298.00	94.1085	0.1525	0.09828	161.364
303.00	101.7870	0.1868	0.09881	133.816
308.00	109.6949	0.2273	0.09935	111.657
313.00	117.7667	0.2748	0.09991	93.714
318.00	125.9718	0.3303	0.10049	79.091
323.00	134.2804	0.3947	0.10108	67.102

With the following abbreviations

Column	Description
T	Temperature
H12	Henry coefficient
PSAT2	Saturated vapor pressure
VL	Liquid volume
VV	Vapor volume

Beside this table several plots are generated. These plots can be printed, saved and copied to the Windows clipboard.

3.1.4 Phase Envelope

The Phase Envelope calculation works only for models with an Equation of State.

Composition

Component	Mole Fractions
11	0.1
31	0.1
1050	0.8


Current Sum: 1

Type: Mole Fractions

The constant concentration for the liquid and vapor phase is defined in the “Composition” box as either mole fractions or weight fractions.

Result

The results are presented in a diagram. It is possible to add the pure vapor pressure curves and the legend by the options at the bottom of the diagram. The exact calculated points can be found in the “Result Grid” Tab. T and P are the temperature and pressure. x1 and y1 are the liquid and vapor phase concentrations of component 1. The volume is represented by v.

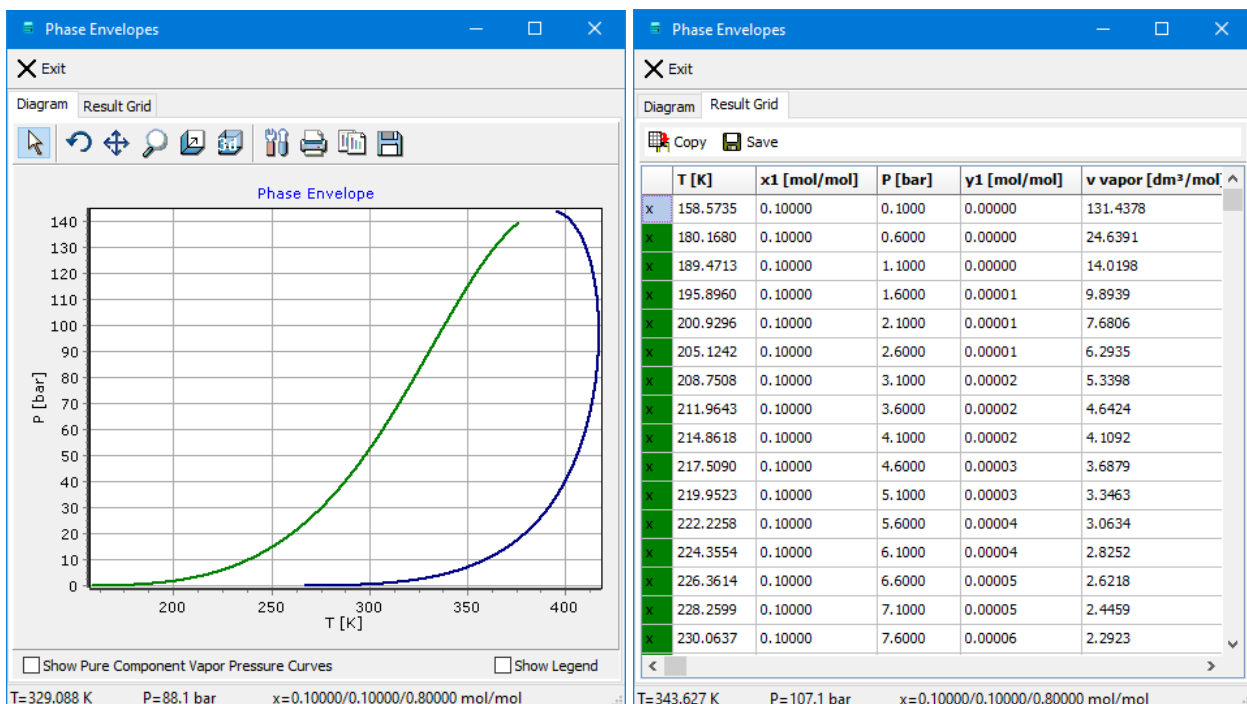

3.2 Solubility

3.2.1 SCF

The SCF (Solubility in supercritical fluid) calculation needs an Equation of State as basis model.

On the right side the calculation temperature is set. The first combo box on the left side specifies the supercritical fluid as solvent for the extraction. Below that, the solute is defined and its associated solid volume and vapor pressure equation. Additionally, a cosolvent can be defined with its concentration in the solvent. At the bottom of the menu, the source of sublimation vapor pressure can be set.

Result

The results are shown after the component and parameter list.

```
Solubility of Carbon dioxide
in supercritical Naphthalene
Co-solvent: Ethanol

Solid volume of solute: 0.1119 dm³/mol

Temperature: 323 K
```

P[bar]	vV[dm³/mol]	y(2)	log(y2)	PHI(2)	POYN(2)	y(1)	y(3)
2.00	13.2935	5.37504733e-04	-3.26962	0.93223	1.00837	0.899462	1.00000000e-01
4.00	6.5790	2.90962049e-04	-3.53616	0.86828	1.01681	0.899709	1.00000000e-01
6.00	4.3402	2.10224811e-04	-3.67732	0.80787	1.02532	0.899790	1.00000000e-01
8.00	3.2204	1.71065323e-04	-3.76684	0.75083	1.03391	0.899829	1.00000000e-01
10.00	2.5480	1.48652297e-04	-3.82783	0.69702	1.04256	0.899851	1.00000000e-01
12.00	2.0995	1.34722540e-04	-3.87056	0.64627	1.05129	0.899865	1.00000000e-01


With the following abbreviations

Column	Description
P	Pressure
VV	Vapor volume
Y2	Vapor mole fraction of component 2
PHI(2)	Fugacity coefficient of component 2
POYN	Poynting factor

Beside this table a diagram is created which shows the logarithmic concentration of the solute against the pressure. This graphic can be saved and copied

3.2.2 SLE

For the SLE (Solid-Liquid Equilibrium) a calculation method has to be chosen from the “Method” Combo Box

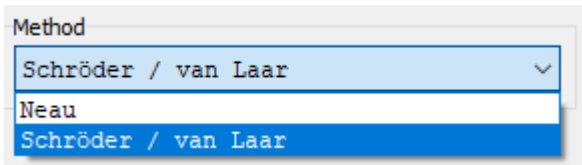


The calculation concentration can be set at the bottom of the menu. The options are similar to the VLE calculation.

Result

The results are shown after the component and parameter list (e.g. Ethanol + Benzene).

T [K]	x1 [1]	x1 [2]
278.68	0.0000	1.0000
278.10	0.0100	0.9900
277.64	0.0200	0.9800
277.26	0.0300	0.9700
276.95	0.0400	0.9600

T is the temperature and x1[1] is the liquid phase concentration of component 1. Additionally, the results are shown as a diagram.

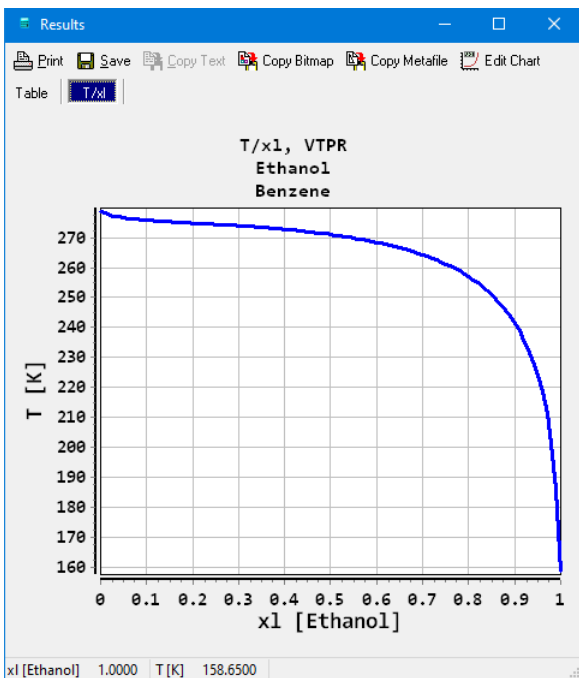

This diagram can be printed, saved or copied. It is also possible to edit the chart.

3.2.3 LLE

The LLE (Liquid-Liquid Equilibrium) calculation works only for binary systems. A temperature range can be set in the menu.

Temperature [K]

Start	End	Step
<input style="width: 80%;" type="text" value="298"/>	<input style="width: 80%;" type="text" value="323"/>	<input style="width: 80%;" type="text" value="5"/>

Pressure [bar]


The pressure is only relevant for calculation with Equation of States.

Result

The results are shown after the component and parameter list (e.g. Water + 1-Butanol).

T [K]	P [bar]	x111	x112	x121	x122
298.00	1.00	0.46371	0.53629	0.98383	0.01617
303.00	1.00	0.46104	0.53896	0.98377	0.01623
308.00	1.00	0.45944	0.54056	0.98367	0.01633
313.00	1.00	0.45883	0.54117	0.98353	0.01647
318.00	1.00	0.45911	0.54089	0.98336	0.01664
323.00	1.00	0.46021	0.53979	0.98316	0.01684

T is the temperature and P is the pressure. x112 is the concentration in phase 1 of component 2. Additionally, the results are shown as adiagram.

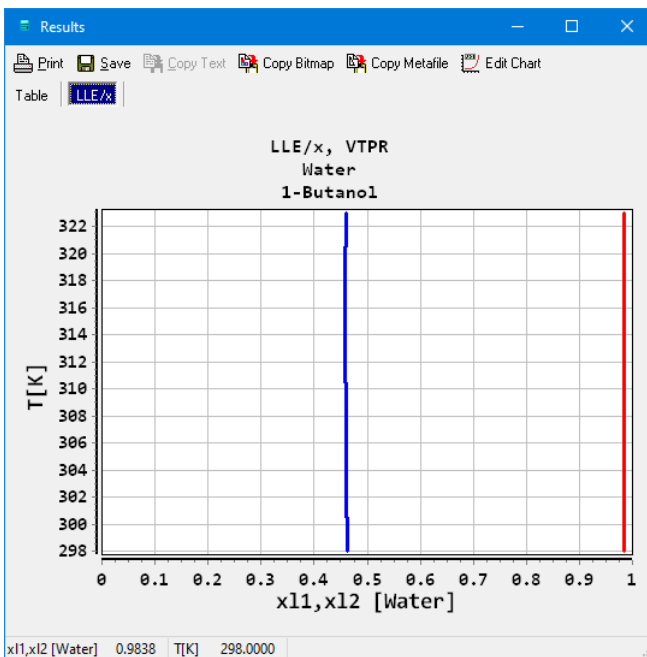


This diagram can be printed, saved or copied. It is also possible to edit the chart.

3.3 Activity

3.3.1 ACT

The ACT (Activity) calculation determines the activity coefficients for given temperatures, pressures and concentrations.

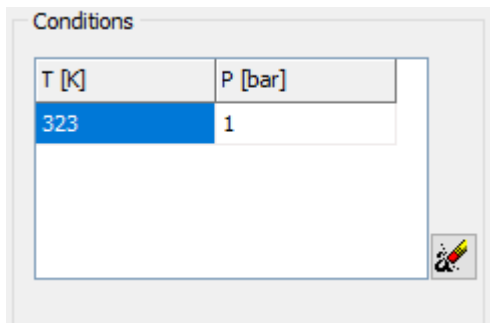


The “Condition” box contains the given calculation temperature and pressure. The concentrations are defined similar to the VLE calculation.

Result

The results are shown after the component and parameter list (e.g., Ethanol + Benzene).

T [K]	P [bar]	x1	x2	gamma1	gamma2
323.00	1.00	0.00000	1.00000	10.56279	1.00000
323.00	1.00	0.01000	0.99000	9.37274	1.00059
323.00	1.00	0.02000	0.98000	8.40178	1.00225
323.00	1.00	0.03000	0.97000	7.59809	1.00483
323.00	1.00	0.04000	0.96000	6.92433	1.00822
323.00	1.00	0.05000	0.95000	6.35310	1.01231
323.00	1.00	0.06000	0.94000	5.86394	1.01704

T is the temperature and P is the pressure. x1 is the concentration of component 1 and gamma1 is the activity coefficient of component 1. Additionally, the results are shown as a diagram.

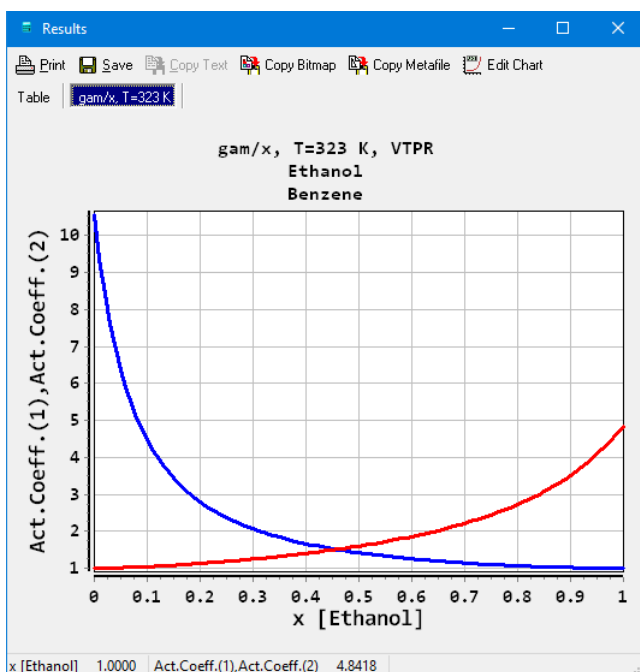

This diagram can be printed, saved or copied. It is also possible to edit the chart.

3.3.2 ACT_inf

The ACT_inf property calculates the activity coefficients of two components at infinite dilution in each other.

Temperature [K]

Start	End	Step
298	323	5

Pressure [bar]

1.


The temperature range has to be set in the menu for the calculation.

Result

The results are shown after the component and parameter list (e.g., Ethanol + Benzene).

T [K]	P [bar]	Actinf1	Actinf2
298.00	1.00	15.95177	5.60115
303.00	1.00	14.61196	5.43918
308.00	1.00	13.42161	5.28256
313.00	1.00	12.36079	5.13097
318.00	1.00	11.41263	4.98414
323.00	1.00	10.56279	4.84182


T is the temperature and P is the pressure. Actinf1 is the activity coefficient of component 1 in infinite dilution in component 2. Additionally there are two further diagrams. The first shows the activity coefficient against the temperature.

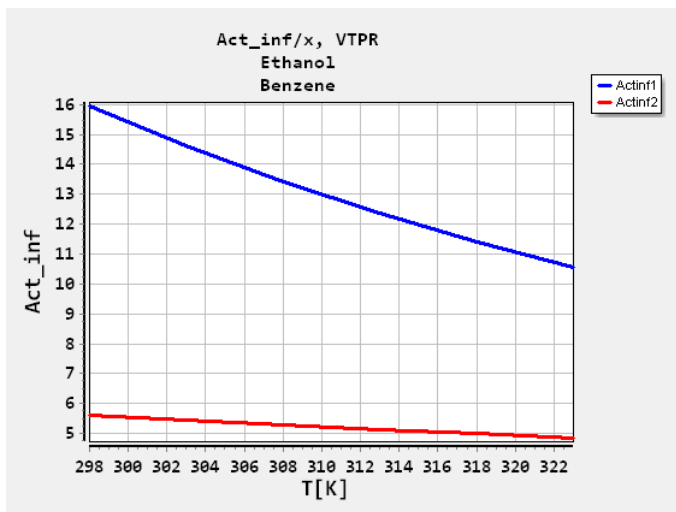

The second graphic is used for an azeotropy estimation. Actinf2 and $1/\text{Actinf1}$ and the quotient of the vapor pressure of component 1 and 2 are shown in the graphic. If the pink line is between the blue and red line azeotropic behavior is given. Is the pink line above or below both other lines the system is zeotropic. If the blue line is above the red line the system shows a positive azeotrope and if the red line is above the blue line the system shows a negative azeotrope.

Positive Azeotrope $\gamma_2^\infty > \frac{p_1^S}{p_2^S} > \frac{1}{\gamma_1^\infty}$

Negative Azeotrope $\gamma_2^\infty < \frac{p_1^S}{p_2^S} < \frac{1}{\gamma_1^\infty}$

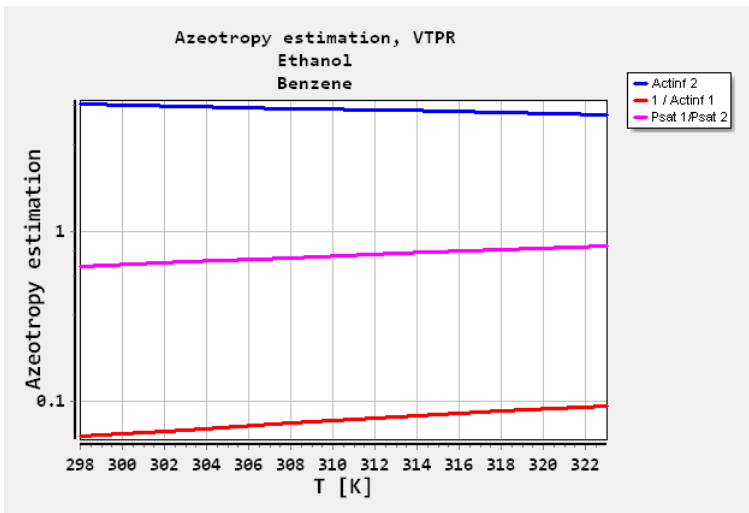

3.3.3 ACT_inf_all

The ACT_inf_all property allows the calculation of the activity coefficients of the system components at infinite dilution in single solvents from a given list. The calculation is also done vice versa.

The calculation temperature and pressure can be set on the left side of the menu. The pressure is only used for calculation with an Equation of State. Normally, the calculation is done for all components of the DDB. This is very time consuming. A list of components can be loaded with the -button. It is also possible to choose a list of solvents with the component selection by using the -button. The Set Range -button opens an extra menu. In this menu a range of components can be selected by using the lowest and highest DDB Number. If the “Check Azeotropy Criterion” is activated, the pure component vapor pressures and an extra azeotropy criterion is calculated in addition to the activity coefficients.

Result

The results are shown in a form of a table for every solvent. Only successful calculations of the activity coefficient are shown.

```

Model: mod. UNIFAC (Dortmund)

List of components:
-----
No.  #DDB  Name
-----
(1)  11  Ethanol


Numbers mark the given components. S marks the tested component
    
```

DDB Nr.	T [K]	Act 1 in S	Act S in 1	Psat 1 [kPa]	Psat S [kPa]	Psat 1/Psat S	AZD 1 S
1	323.00	0.932942	0.963623	29.2128	266.048	0.109803	None Acetaldehyde
2	323.00	0.889133	0.883587	n.a.	n.a.	n.a.	n.a. Acetamide
3	323.00	3.10404	3.4345	29.2128	33.6225	0.868846	Positive Acetonitrile
4	323.00	1.95287	2.09795	29.2128	81.1996	0.359765	None Acetone
5	323.00	0.278885	0.0399946	29.2128	6.79191	4.30112	None Ethylenediamine
6	323.00	7.21078	4.66812	29.2128	5.49039	5.32071	None 1,2-Dibromoethane
7	323.00	11.0551	3.74572	29.2128	148.291	0.196996	Positive Ethyl bromide
8	323.00	1.31162	1.31277	29.2128	0.0908638	321.5	None 1,2-Ethanediol
9	323.00	12.1836	5.31729	29.2128	48.0086	0.60849	Positive Ethyl iodide
10	323.00	1.29166	2.22234	29.2128	0.0216487	1349.4	None 5-Ethyl-2-nonanol
12	323.00	4.22292	3.15011	29.2128	170.142	0.171696	None Diethyl ether
13	323.00	0.999729	0.878719	29.2128	390.027	0.0748994	None Ethylene oxide
14	323.00	1.06127	1.0864	29.2128	13.243	2.2059	None 2-Propen-1-ol
16	323.00	3.06495	3.14298	29.2128	86.8486	0.336364	Positive Formic acid ethyl ester
17	323.00	2.53841	3.15101	29.2128	0.436643	66.9031	None Aniline
18	323.00	3.53589	4.06319	29.2128	2.03598	14.3483	None Methoxybenzene
19	323.00	1.06865	1.70422	29.2128	5.56974	5.2449	None 2-Methylpyridine
20	323.00	16.0316	7.44499	29.2128	2.34534	12.4557	None .alpha.-Pinene
21	323.00	2.35463	2.37148	29.2128	37.6684	0.775524	Positive Ethyl acetate
22	323.00	1.08289	1.12209	29.2128	10.8736	2.68659	None 2-Butanol

The table uses the following abbreviations


Column	Description
T	Temperature
Act 1 in S	Activity Coefficient of component 1 at infinite dilution in the solvent
Act S in 1	Activity Coefficient of the solvent in infinite dilution in component 1
Psat 1	Vapor pressure of component 1
AZD 1 S	Azeotropic behavior in the system component 1 with the solvent (explanation see chapter Act_inf)
n.a.	Vapor pressure is missing

Activity coefficient pairs are displayed in a diagram. The solvent information of every point is with its values at the bottom.

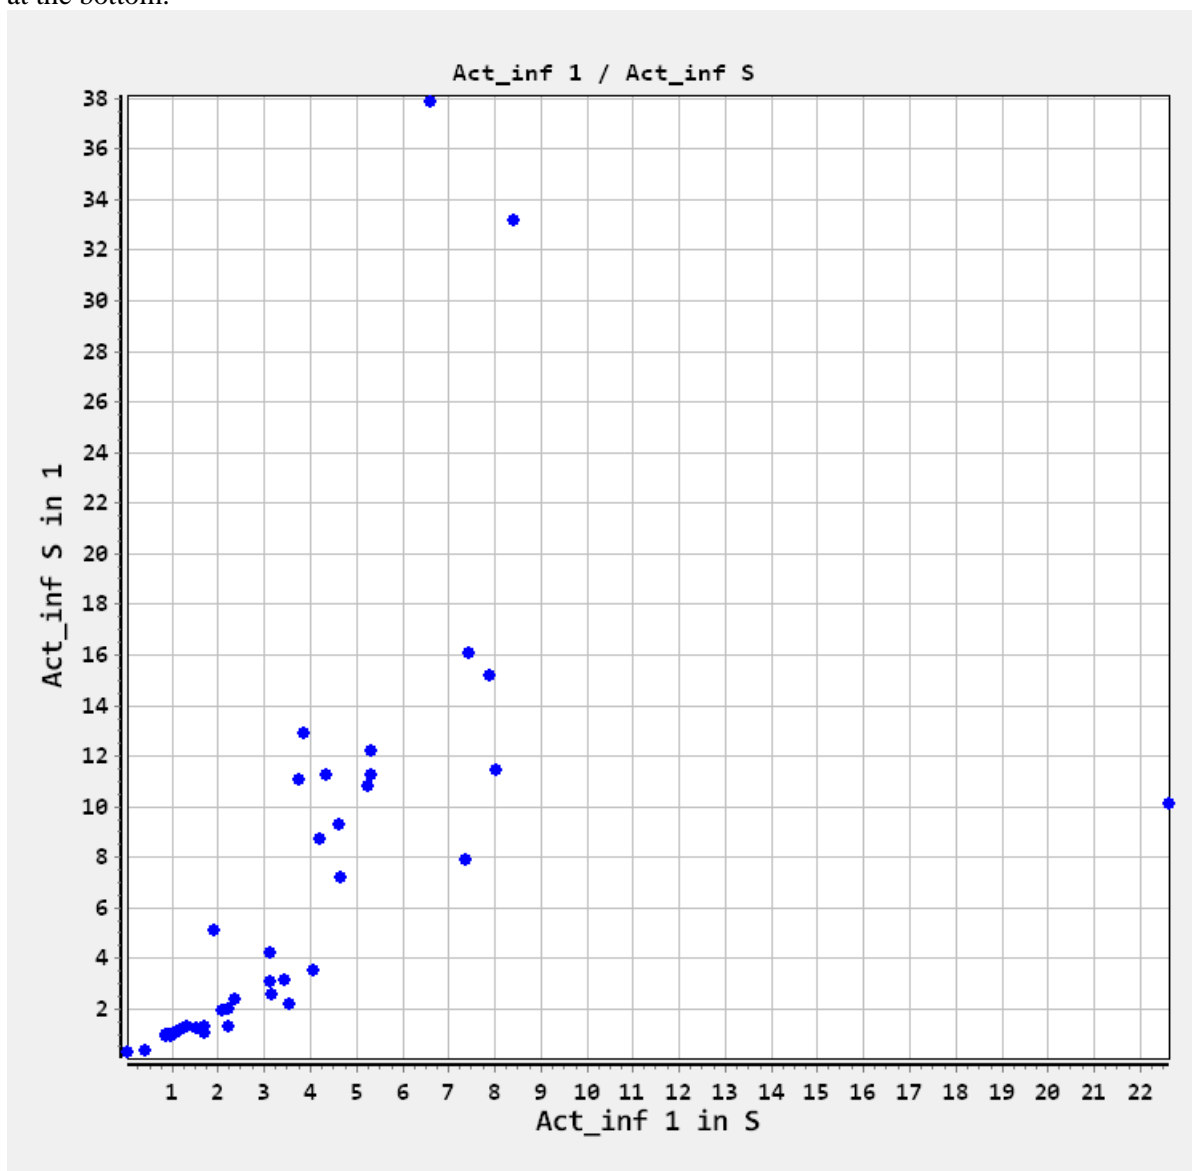

3.4 Excess properties

All excess properties have very similar calculation options. Under “Conditions” it is possible to define calculation temperatures and calculation pressures for models with an equation of state.

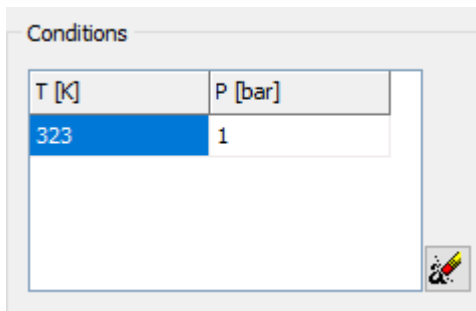

At the bottom, the concentrations can be defined for the calculation. The handling is very similar to the VLE options.

3.4.1 HE


This property calculates the excess enthalpies for a given system. This calculation is possible with all models. However, the pressure is only used for models with an equation of state.

Result

The results are shown after the component and parameter list.

T [K]	P [bar]	hE [J/mol]	x1	x2
323.00	1.00	0.00	0.00000	1.00000
323.00	1.00	125.13	0.01000	0.99000
323.00	1.00	237.54	0.02000	0.98000
323.00	1.00	339.03	0.03000	0.97000
323.00	1.00	431.08	0.04000	0.96000

T is the temperature, P is the pressure and hE the excess enthalpy. For each component, the liquid concentration is given as x. Additionally the results are shown as a diagram.

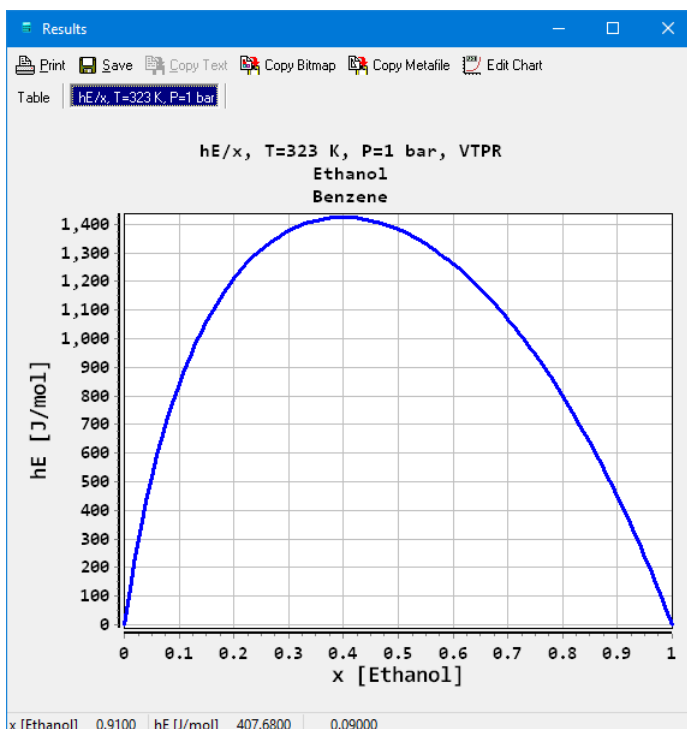

This diagram can be printed, saved or copied. It is also possible to edit the chart.

3.4.2 VE


Excess volumes can only be calculated by models with an equation of state.

Result

The results are shown after the component and parameter list.

T [K]	P [bar]	vE [cm ³ /mol]	x1	x2
323.00	1.00	0.0000	0.00000	1.00000
323.00	1.00	0.0577	0.01000	0.99000
323.00	1.00	0.1121	0.02000	0.98000
323.00	1.00	0.1635	0.03000	0.97000
323.00	1.00	0.2120	0.04000	0.96000

T is the temperature, P is the pressure and vE the excess volume. For each component, the liquid concentration is given as x. Additionally the results are shown as a diagram.

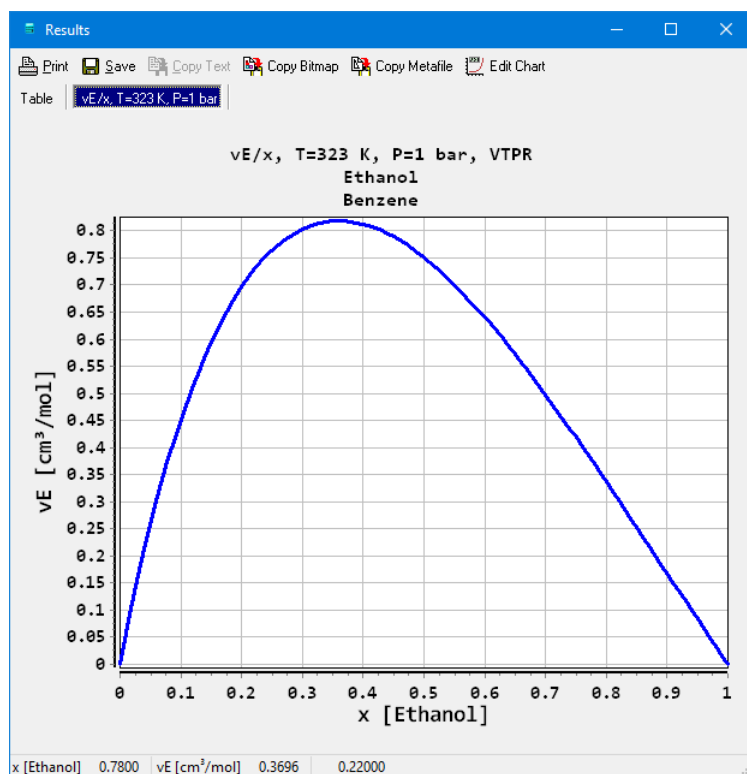

This diagram can be printed, saved or copied. It is also possible to edit the chart.

3.4.3 CPE


This property calculates the excess heat capacities for a given system. This calculation is possible with all models. However, the pressure is only used for models with an equation of state.

Result

The results are shown after the component and parameter list.

T [K]	P [bar]	cpE [J/mol/K]	x1	x2
323.00	1.00	0.0000	0.00000	1.00000
323.00	1.00	0.0883	0.01000	0.99000
323.00	1.00	0.2982	0.02000	0.98000
323.00	1.00	0.5912	0.03000	0.97000
323.00	1.00	0.9396	0.04000	0.96000

T is the temperature, P is the pressure and cpE the excess heat capacity. For each component, the liquid concentration is given as x. Additionally the results are shown as a diagram.

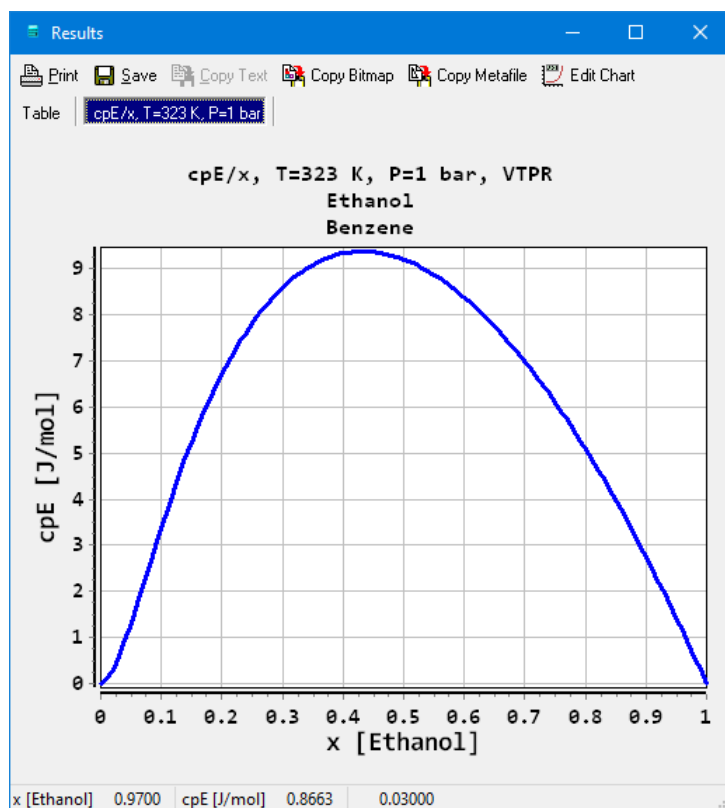

This diagram can be printed, saved or copied. It is also possible to edit the chart.